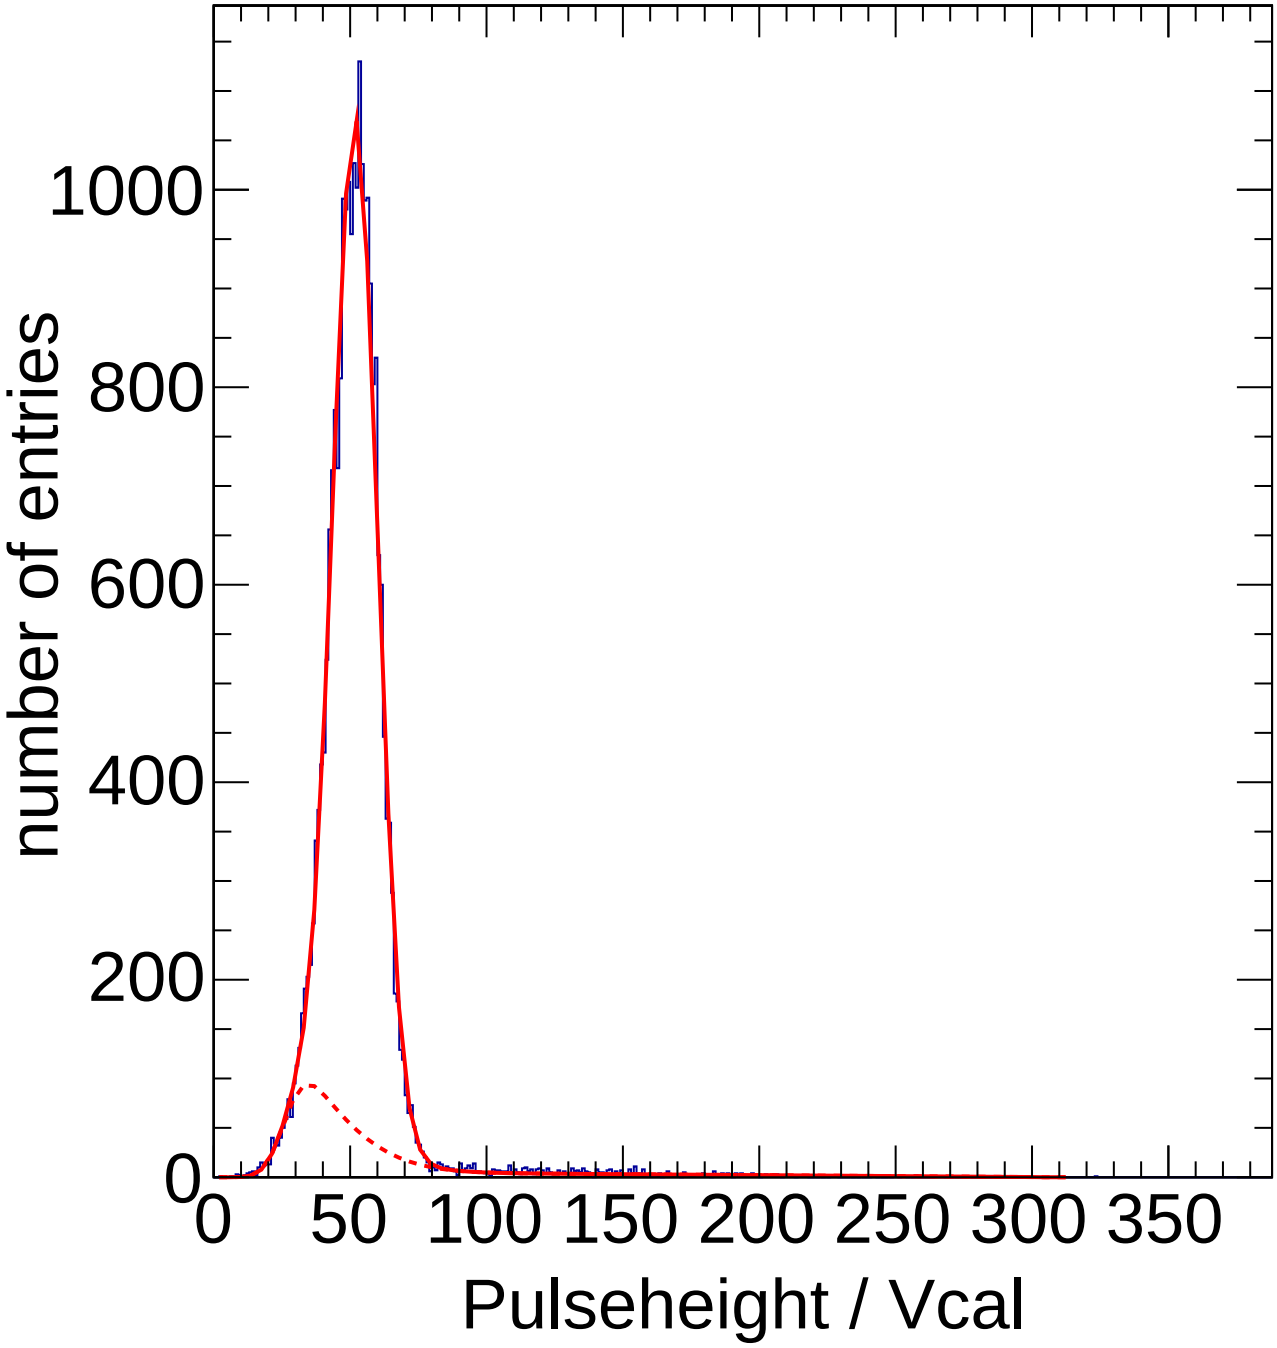X-ray Calibration - Target Zn Method Spectrum Chip C12