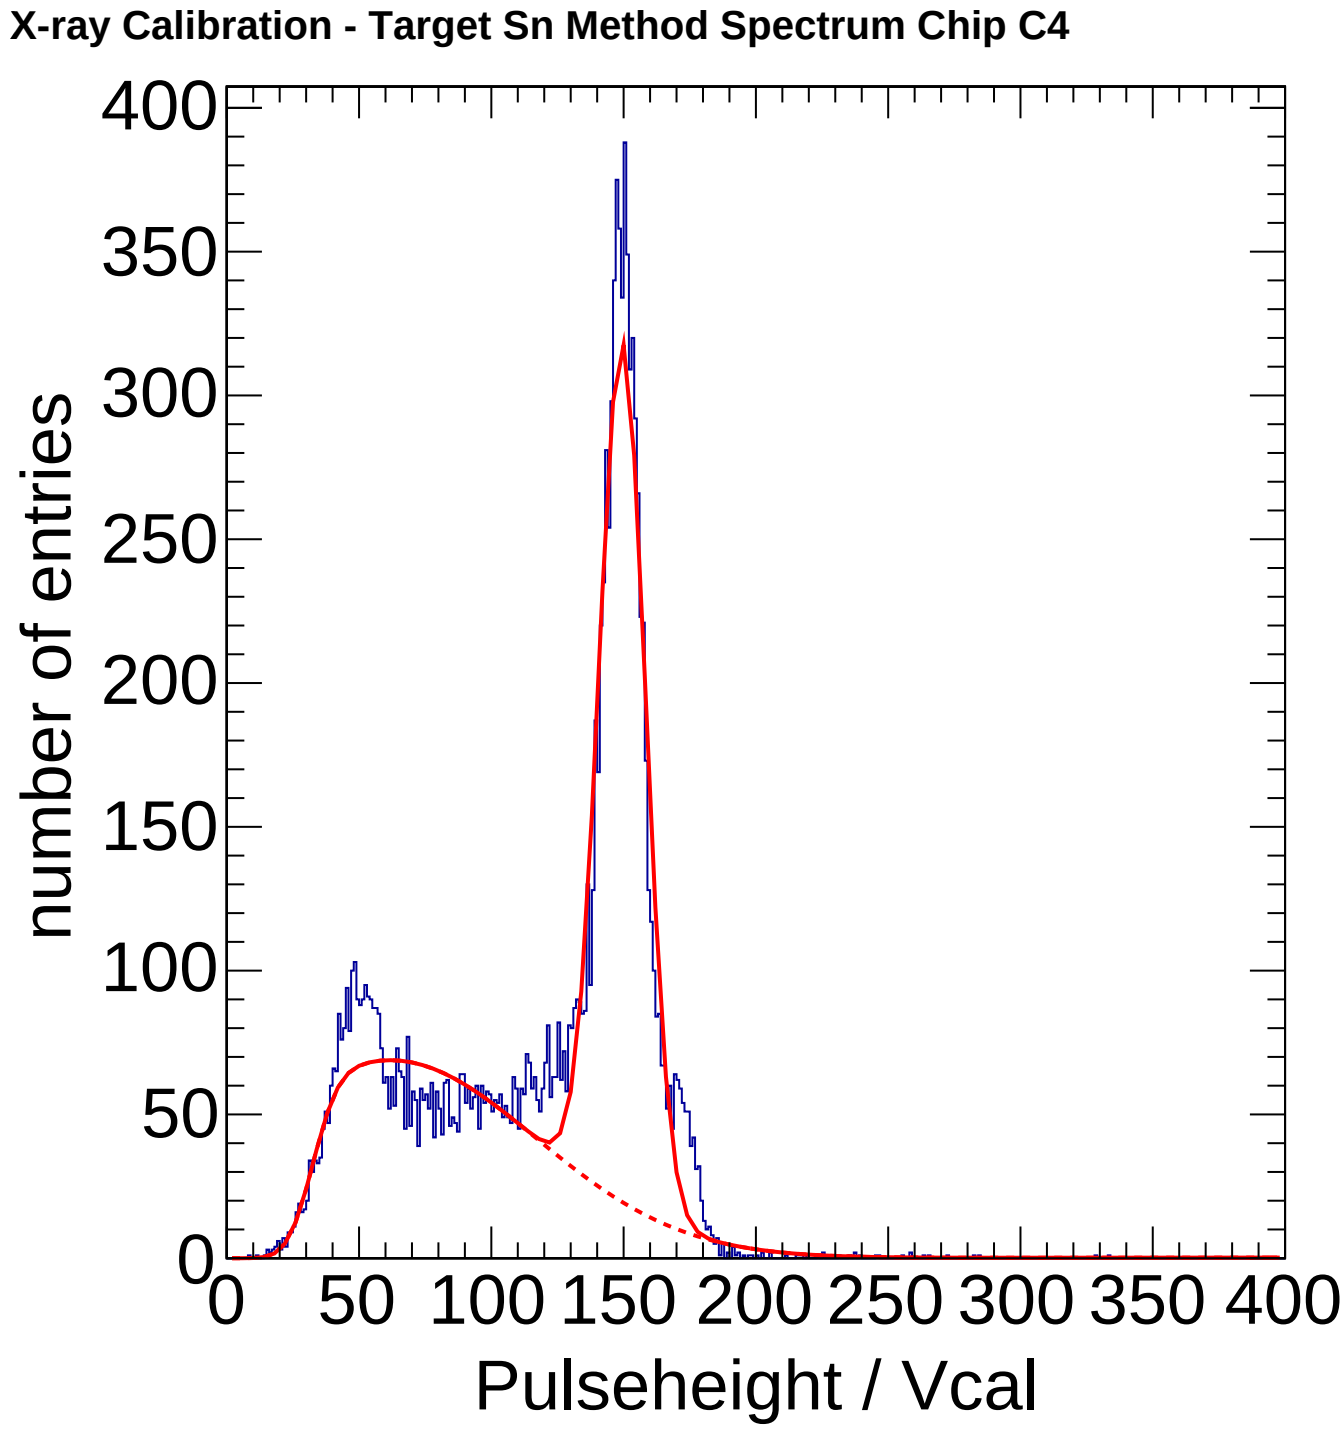
X-ray Calibration - Target Sn Method Spectrum Chip C4
number of entries
Pulseheight / Vcal
0
50
100
150
200
250
300
350
400