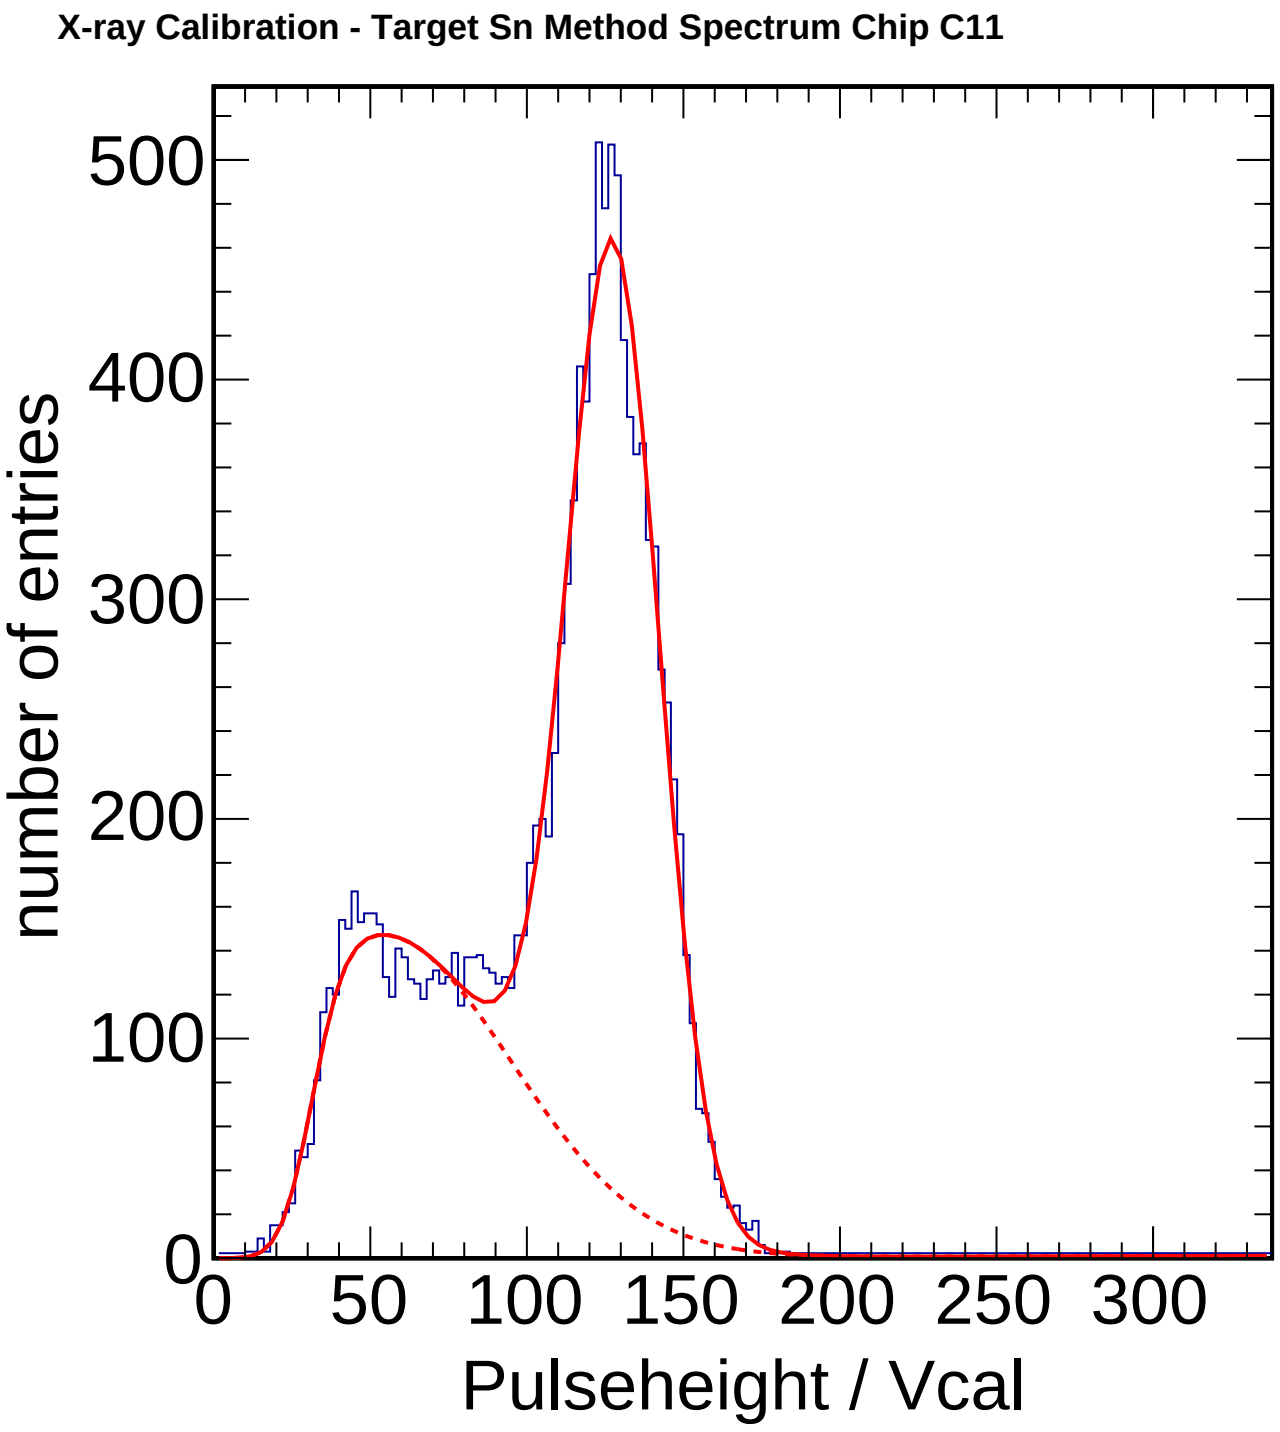
X-ray Calibration - Target Sn Method Spectrum Chip C11
number of entries
0
100
200
300
400
500
0
50
100
150
200
250
300
Pulseheight / Vcal